

Comparison of Central, Peripheral and Weighted Size Specific Dose in CT to Dose Results from IndoseCT Software

by Eko Hidayanto

Submission date: 14-Jul-2022 07:40AM (UTC+0700)

Submission ID: 1870252337

File name: e_Specific_Dose_in_CT_to_Dose_Results_from_IndoseCT_Software.pdf (292.34K)

Word count: 2750

Character count: 13678

Comparison of Central, Peripheral and Weighted Size Specific Dose in CT to Dose Results from IndoseCT Software

Putryani Dio, Choirul Anam, Eko Hidayanto

Department of Physics, Diponegoro University, Semarang, Indonesia

Corresponding author: Eko Hidayanto

DOI: <https://doi.org/10.52403/ijrr.20220729>

8

ABSTRACT

The purpose of this study was to calculate the average dose of a phantom with a diameter of 16 and 32 cm, as well as the dose distribution in the center and periphery. The results were then compared to those from the IndoseCT software. In this study, a standard PMMA phantom with a diameter variation of 16 and 32 cm was used. The phantom was scanned using fixed parameters, namely 120 kVp voltage, 100 mAs time current, 10 mm collimation width, 100 mm scan length, and 1 s tube rotation. This research was conducted at the Indriati Solo Baru Hospital using the GE CT scanner type Revolution EVO 64/128 slice. The results of this study show that for a 16 cm phantom diameter at the center position the difference in detector measurements with IndoseCT is 1.34% at the phantom edge position is 4.38% and the weighted dose is 2.59 %, while for a 32 cm phantom diameter, the difference is 8.1 percent, at the edge of the phantom it is 1.26 %, and the weighted dose is 0.62 %. Based on the results obtained from IndoseCT, it showed an insignificant difference with the measurement of radiation dose using a phantom. Overall, the difference in percentage is $\pm 10\%$ while the difference in percentage that is still acceptable is $\pm 20\%$.

Keywords: Pencil ion chamber, PMMA phantom, dose distribution, size-specific dose estimate (SSDE), central dose, peripheral dose, weighted dose, IndoseCT 20.b.

INTRODUCTION

The internal organs of the human body are examined using x-rays by the diagnostic assistance tool known as a computed tomography (CT) scan [1,2]. CT scans are widely used in clinical examinations because

they have high radiographic contrast so that the available contrast from CT scan images is far superior to conventional radiography [3]. The dose on CT scan is very large when compared to conventional radiology modalities. The relatively higher doses on CT scans have the potential to pose risks to people undergoing CT scans [4]. To overcome this problem, it is necessary to measure the amount of radiation dose received by the patient and released by the device [5,6].

Computed Tomography Dose Index (CTDI) is a quantity used to calculate the quantity of radiation in determining the dose received by a patient on a CT scan. CTDI measurements are usually performed using a standard phantom polymethyl methacrylate (PMMA), which has a diameter of 16 cm to represent the patient's head and a diameter of 32 cm to represent the patient's body with a length of 14 to 15 cm [6,7]. The CT scan dose is expressed in terms of the CTDI volume (CTDIvol), whereas this metric only shows the radiation output of the CT scan [7,8]. Due to this, the American Association of Physicists in Medicine (AAPM) in 2011 released Report No. 204 about the dose in patients undergoing a CT scan. This report describes the Size Specific Dose Estimate (SSDE), which is computed using the CTDI value and the conversion factor (f) obtained from the effective diameter of the patient or the patient's body size [9]. However, the dose received by the patient is also influenced by the ct scan radiation output (ie kV, mAs, pitch, rotation time and collimation

width), also determined by the characteristics of each individual patient [10]. Therefore, the American Association of Physicists in Medicine (AAPM) published Report No. 220 in 2014 to determine SSDE based on individual patient characteristics, also known as water equivalent diameter (D_w) [11]. The SSDE value can also be determined automatically by the IndoseCT software, which makes it simpler for users to determine the SSDE value, in addition to being determined from direct measurements [12].

Anam *et al* [13] conducted a study to calculate several organ doses, namely liver and kidney using the SSDE concept and compared the results with the doses calculated using the Monte Carlo method. The percentage difference between the doses of the proposed method and the Monte Carlo method was 5.47% in the liver, 21.77% in the right kidney and 22.64% in the left kidney, respectively.

The purpose of this study was to measure the value of the dose distribution in the center, the edge of the phantom, and the average dose of the phantom with a diameter of 16 and 32 cm and then the results were compared with the values obtained in the IndoseCT software.

METHODS AND MATERIAL

This study was carried out at the Indriati Solo Baru Hospital. The fixed parameters used are 120 kVp tube voltage, 100 mAs time current, 10 mm collimation width, 100 mm scan length, and 1 s tube rotation.

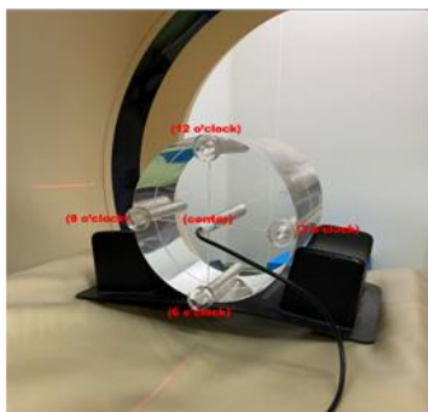


Figure 1. Detector position for CTDI measurement

This research was conducted using a pencil ion chamber and a PMMA phantom with

a diameter of 16 and 32 cm. The phantom is positioned precisely according to the horizontal and vertical laser crossing. The Pencil Ion Chamber is placed in the center of the phantom to obtain the CTDI_{center} (CTDI_c) value. While the pencil ion chamber is placed on the four edges of the phantom to get the CTDI peripheral (CTDI_p) value (figure 1).

This measurement was carried out 15 times scanning for each phantom with fixed parameters so that the total measurement was 30 scanning times because 3 measurements were carried out for each phantom hole. The phantom image is stored in a DICOM file. The data were processed using the IndoseCT 20.b to calculate the dose values for one phantom center hole and four phantom edges for 16 and 32 cm phantom diameters, respectively.

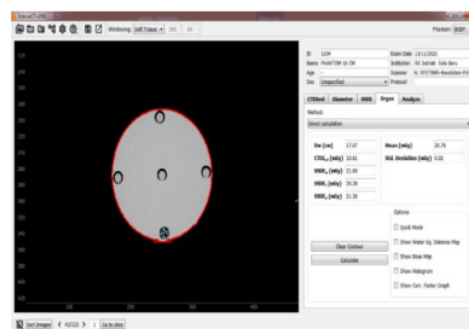


Figure 2. Contouring organs of CTDI phantom

The IndoseCT 20.b calculated the dose in phantoms with diameter variations of 16 and 32 cm using interpolation between the central SSDE (SSDE_c) and the four phantom periphery (SSDE_p). The calculation begins with the contouring of the organ manually. Organ contours aim to determine the location and area of the organ that will be used to measure the average dose of the organ and its standard deviation. In this software, organ contouring cannot be performed for two organs simultaneously, so the contouring process is carried out for each organ. The contour was carried out 10 times for each variation of the 16 and 32 cm phantom because each had 5 phantom holes, namely the middle hole and four at the edges of the phantom (Figure 2).

The SSDE value was calculated from the measurements made for each hole, one measurement on the center hole (SSD_c) and four

on each side of the phantom edge (SSDE_p). The SSDE_c and SSDE_p for estimating phantom organs dose distribution can be calculated based on the conversion coefficient (k and h) and CTDI_w Eq (1) (2).

$$SSDE_c = h \times CTDI_w \quad (1)$$

$$SSDE_p = k \times CTDI_w \quad (2)$$

The SSDE weight values (SSDE_w) were computed using the SSDE_c and SSDE_p values as a function of the equivalent diameter based on Eq (3).

$$SSDE_w = f_w \times \frac{CTDI_w}{pitch} \quad (3)$$

Conversion factors h and k have been stored in IndoseCT 20.b. Thus, when calculating the dose distribution, it will be calculated automatically by the indosect 20.b as shown in figure 2. After obtaining the measured radiation dose values on the surface and the four phantom edges as well as the radiation dose value from IndoseCT 20.b then calculate the percentage difference based on Eq (4).

$$\% \text{ Difference} = \frac{A-B}{A} \times 100\% \quad (4)$$

With A indicating the CTDI value measured in phantom and B indicating the CTDI value calculated using the IndoseCT 20.b.

RESULTS AND DISCUSSION

This study aimed to compare the dose measured directly with the dose calculated from IndoseCT 20.b using standard phantom diameter variations of 16 and 32 cm both in the center of the phantom and at the periphery of the phantom. This research was conducted at Indriati Solo Baru Hospital using the GE CT scanner Revolution EVO 64/128 slice type. This research was conducted using fixed parameters, namely tube voltage 120 kVp, current 100 mAs, collimation width 10 mm, scan length 100 mm, and tube rotation 1 s.

Dose measurement with a Pencil Ion Chamber

The results of the dose measurement on the PMMA phantom showed that the dose values in the center of the phantom were 20.01 and 6.57 mGy, the peripheral were 22.34 and 13.48 mGy, and the weighted dose values were 21.56 and 11.17 mGy for phantoms with diameters of 16 and 32 cm, respectively.

The dose value at the five detector placement positions is inversely proportional to the variation of the phantom diameter. In this case, the phantom with a diameter of 32 cm produces a smaller radiation dose compared to the radiation dose at the edge of the phantom. The radiation dose ratio at the four edges of the phantom hole is almost the same value, while at the phantom center the radiation dose value is the lowest.

Dose Calculations Using IndoseCT 20.b

The results shown on the IndoseCT software are 20.28 mGy and 7.10 mGy for the dose values in the central position, 21.36 mGy and 13.31 mGy for the dose values at the periphery of the phantom, and 21.00 mGy and 11.24 mGy for the weighted dose with phantom diameters of 16 cm and 32 cm, respectively.

Comparison of phantom measurement dose values with IndoseCT 20.b

Figure 3 shows the comparison between the dose value from the IndoseCT software and the dose on the radiation detector. The dose difference for a 16 cm diameter phantom in the center position was 1.34%; at the periphery of the phantom position of 4.38% and the weighted dose was 2.59%; and for the 32 cm phantom diameter, the dose difference was 8.1% at the center position, 1.26% at the periphery position, and 0.62% at the weighted dose.

Figure 3(a) shows a graph with almost the same graphic appearance between measurements using a detector with IndoseCT software. The SSDE_c dose value from the detector measurement has a smaller dose value compared to the dose result in the IndoseCT software. The difference in percentage between the two is the largest 8.1% in the center position of the phantom with the diameter of the phantom is 32 cm. Figure 3 (b) shows a graph of the comparison of dose values on the edge of the phantom with IndoseCT software showing almost the same pattern. For a phantom diameter of 16 cm, the percentage difference is greater than that of a phantom diameter of 32 cm. For Figure 3 (c) the value of the weighted dose at a phantom diameter of 32 cm, the percentage difference is very small, namely 0.62%.

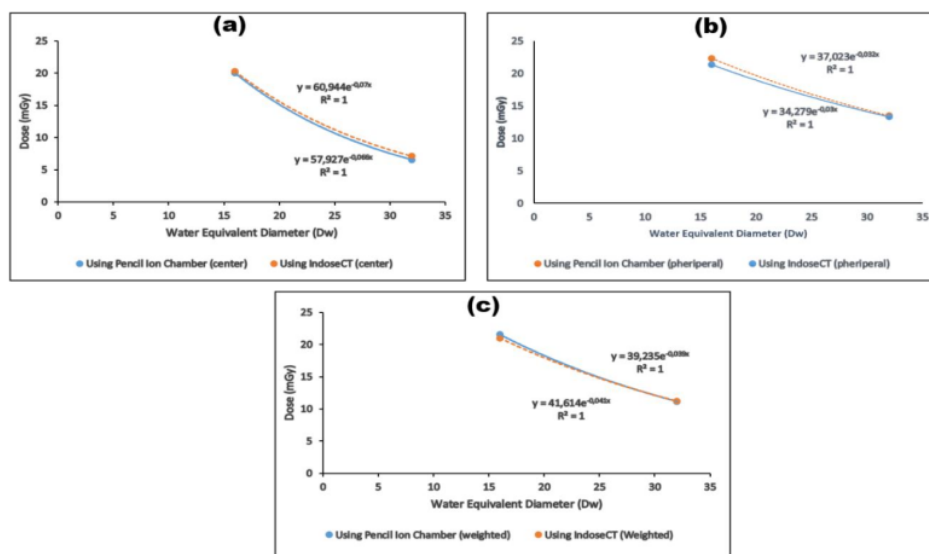


Figure 3. Graph of dose comparison on phantom with IndoseCT software on (a) SSDc (b) SSDEp (c) SSDEw

13 In this work, the radiation dose was measured using a pencil-shaped ion chamber detector with PMMA phantoms that varied in diameter from 16 to 32 cm. This measurement was carried out to compare the dose results from the IndoseCT software to the dose correlation in each phantom hole using a pencil ion chamber. The increase in the phantom diameter is inversely proportional to the dose value. This indicates that the measured dose value decreases as the phantom diameter increases. In comparison to the 32 cm phantom diameter, the 16 cm phantom diameter has the highest dose value. The results obtained indicate that the difference in results is almost the same between direct measurements in each phantom hole and the dose results in the IndoseCT software. According to AAPM 204, the diameter variation from various methods can only reach 16% for small diameters [9]. Therefore, AAPM recommends an acceptable SSDE limit of 20% [9].

15 CONCLUSION

The results of this study show that for a 16 cm phantom diameter at the center position, the difference in the percentage of detector measurements with IndoseCT software is 1.34%, at the phantom edge position, it is 4.38%, and the weighted dose is 2.59%, while

for a 32 cm phantom diameter, the difference is 8.1 percent, at the edge of the phantom it is 1.26 %, and the weighted dose is 0.62 %.

Based on the results obtained from IndoseCT, it showed an insignificant difference with the measurement of radiation dose using a phantom. Overall, the difference in percentage is $\pm 10\%$ while the difference in percentage that is still acceptable is $\pm 20\%$.

Acknowledgement: None

Conflict of Interest: None

Source of Funding: None

REFERENCES

1. Karatas OH and Toy E. Three dimensional imaging techniques: A literature review. *Eur J Dent.* 2014; 8(1): 132–140.
2. Manmadhacharya A, Kumar YR, Krishnananda L., Effect of CT acquisition parameters of spiral CT on image quality and radiation dose *Measurement.* 2017; 103: 18–26.
3. INTERNATIONAL ATOMIC ENERGY AGENCY, *Quality Assurance Programme for Computed Tomography: Diagnostic and Therapy Applications*, Human Health Series, Vienna; 2012

4. Turner AC, *et al.* The feasibility of a scanner-independent technique to estimate organ dose from MDCT scans: Using CTDI vol to account for differences between scanners. *Med Phys.* 2010;37(4):1816-1825.
5. Anam, C., Haryanto, F., Widita, R., Arif, I., Dougherty, G., 2016a, A fully automated calculation of size-specific dose estimates (SSDE) in thoracic and head CT examinations. *Journal of Physics Conference Series*, Vol 694, Conference 1.
6. Anam, C., Haryanto, F., Widita, R., Arif, I., dan Dougherty, G., 2016, Automated Calculation Of Water-Equivalent Diameter (D_w) Based On Aapm Task Group 220, *Journal Of Applied Clinical Medical Physics*, Volume 17, Number 4.
7. Anam C, Haryanto F, Widita R, Arif I, and Dougherty G 2017 The evaluation of the effective diameter (D_{eff}) calculation and its impact on the size-specific dose estimate (SSDE) *Atom Indonesia* 43 55-60
8. Bauhs JA, Vrieze T, Primak A, Bruesewitz M, McCollough CH. *CT Dosimetry: Comparison of Measure Techniques and Devices*. Radiological Society of North America. 2008-28:246-252.
9. American Association of Physicists in Medicine.. 2011, Size specific dose estimates (SSDE) in pediatric and adult body CT examinations report no. 204, doi:www.aapm.org/pubs/reports/rpt_204. pdf Accessed February 05, 2021.
10. Anam, C., Haryanto, F., Widita, R., Arif, I., dan Dougherty, G., 2017, The Size Specific Dose Estimate (SSDE) For Truncated Computed Tomography Images. *Radiation Protection Dosimetry*, Vol.175, No.3, pp.313-320.
11. Anam, C., Haryanto, F., Widita, R., Arif, I., dan Dougherty, G., 2016, Automated Calculation Of Water-Equivalent Diameter (D_w) Based On Aapm Task Group 220, *Journal Of Applied Clinical Medical Physics*, Volume 17, Number 4.
12. Anam C., *et al.* Indose CT: Software for calculating and Managing Radiation Dose of Computed Tomography for an Individual Patient Manual-Version 20.b, Agustus 2021.
13. Anggraini MH and Anam C. Dose Estimations of Kidney and Liver on Abdominal CT Examination Based on Size-Specific Dose Estimation (SSDE). *Journal of Physics: Conference Series*.2021.
14. RTI Electronics, 2009, *CT dose profile analyzer manual version 4.0B*. Sweden: RTI Electronics.

How to cite this article: Putryani Dio, Choirul Anam, Eko Hidayanto. Comparison of central, peripheral and weighted size specific dose in CT to dose results from IndoseCT software. *International Journal of Research and Review*. 2022; 9(7): 249-253. DOI: <https://doi.org/10.52403/ijrr.20220729>

Comparison of Central, Peripheral and Weighted Size Specific Dose in CT to Dose Results from IndoseCT Software

ORIGINALITY REPORT

12%

SIMILARITY INDEX

5%

INTERNET SOURCES

11%

PUBLICATIONS

1%

STUDENT PAPERS

PRIMARY SOURCES

1

ijamscr.com

Internet Source

1%

2

"Report 87", Journal of the ICRU, 2012.

Publication

1%

3

Jan Juszczuk, Pawel Badura, Joanna Czajkowska, Agata Wijata et al. "Automated size-specific dose estimates using deep learning image processing", Medical Image Analysis, 2021

Publication

1%

4

Medical Radiology, 2012.

Publication

1%

5

Rakhma Noviliawati, Choirul Anam, Heri Sutanto, Geoff Dougherty, Muhammad Ridha Mak'ruf. "Automatic validation of the gantry tilt in a computed tomography scanner using a head polymethyl methacrylate phantom", Polish Journal of Medical Physics and Engineering, 2021

Publication

1%

6	Michael J. Dennis. "Computed Tomography", Wiley, 2006 Publication	1 %
7	Madan Rehani. "Chapter 2 Radiation Units, Limits and Dose Constraints", Springer Science and Business Media LLC, 2011 Publication	1 %
8	academic.oup.com Internet Source	<1 %
9	www.jacmp.org Internet Source	<1 %
10	Anam, C, F Haryanto, R Widita, I Arif, and G Dougherty. "Profile of CT scan output dose in axial and helical modes using convolution", Journal of Physics Conference Series, 2016. Publication	<1 %
11	Martin Caon, Giovanni Bibbo, John Pattison, Madhava Bhat. "The effect on dose to computed tomography phantoms of varying the theoretical x-ray spectrum: A comparison of four diagnostic x-ray spectrum calculating codes", Medical Physics, 1998 Publication	<1 %
12	Jenia Vassileva, Madan M. Rehani, Kimberly Applegate, Nada A. Ahmed, Humoud Al-Dhuhli, Huda M. Al-Naemi. "IAEA survey of paediatric computed tomography practice in	<1 %

40 countries in Asia, Europe, Latin America and Africa: procedures and protocols",
European Radiology, 2012

Publication

13

John M. Boone. "The trouble with CTDI100",
Medical Physics, 2007

Publication

<1 %

14

Sigal Trattner, Anjali Chelliah, Peter Prinsen,
Carrie B. Ruzal-Shapiro et al. "Estimating
Effective Dose of Radiation From Pediatric
Cardiac CT Angiography Using a 64-MDCT
Scanner: New Conversion Factors Relating
Dose-Length Product to Effective Dose",
American Journal of Roentgenology, 2017

Publication

<1 %

15

Ceinos, Romain, Delphine Tardivo, Marie-
France Bertrand, and Laurence Lupi-Pegurier.
"Inter- and Intra-Operator Reliability of Facial
and Dental Measurements Using 3D-
Stereophotogrammetry : INTER- AND INTRA-
OPERATOR RELIABILITY OF FACIAL AND
DENTAL MEASUREMENTS", Journal of Esthetic
and Restorative Dentistry, 2016.

Publication

<1 %

16

Choirul Anam, Idam Arif, Freddy Haryanto,
Rena Widita, Fauzia P Lestari, Kusworo Adi,
Geoff Dougherty. "A SIMPLIFIED METHOD
FOR THE WATER-EQUIVALENT DIAMETER

<1 %

CALCULATION TO ESTIMATE PATIENT DOSE IN CT EXAMINATIONS", Radiation Protection Dosimetry, 2019

Publication

17

ijrr.com

Internet Source

<1 %

18

pubs.rsna.org

Internet Source

<1 %

19

Choirul Anam, Freddy Haryanto, Rena Widita, Idam Arif, Geoff Dougherty, Donald McLean. "The impact of patient table on size-specific dose estimate (SSDE)", Australasian Physical & Engineering Sciences in Medicine, 2016

Publication

<1 %

20

Kevin Treb, Ke Li. "Accuracy of weighted CTDI in estimating average dose delivered to CTDI phantoms: An experimental study", Medical Physics, 2020

Publication

<1 %

21

Marcel van Straten, Paul Deak, Paul C. Shrimpton, Willi A. Kalender. "The effect of angular and longitudinal tube current modulations on the estimation of organ and effective doses in x-ray computed tomography", Medical Physics, 2009

Publication

<1 %

22

Keith J. Strauss. "KERMA ratios vs. SSDE: is one better at estimating pediatric CT radiation doses?", *Pediatric Radiology*, 2012

Publication

<1 %

23

M'hamed El Mansouri, Abdelmajid Choukri, Slimane Semghouli, Mohammed Talbi, Khalida Eddaoui, Zouhir Saga. "Size-Specific Dose Estimates for Thoracic and Abdominal Computed Tomography Examinations at Two Moroccan Hospitals", *Journal of Digital Imaging*, 2022

Publication

<1 %

Exclude quotes Off

Exclude matches Off

Exclude bibliography On