

An artifact-free thyroid shield in CT examination a phantom study

by Heri Sutanto

Submission date: 26-Feb-2023 01:27PM (UTC+0700)

Submission ID: 2023097468

File name: tifact-free_thyroid_shield_in_CT_examination_a_phantom_study.pdf (998.88K)

Word count: 4984

Character count: 24048

Biomedical Physics & Engineering Express



PAPER

An artifact-free thyroid shield in CT examination: a phantom study

RECEIVED
13 November 2019REVISED
17 January 2020ACCEPTED FOR PUBLICATION
22 January 2020PUBLISHED
31 January 2020Heri Sutanto¹, Yulia Irdawati¹, Choirul Anam¹, Toshioh Fujibuchi², Geoff Dougherty³,
Eko Hidayanto¹, Zaenal Arifin¹, Johny Wahyuadi Soedarsono⁴ and Bahrudin⁵¹ Department of Physics, Faculty of Sciences and Mathematics, Diponegoro University, Jl. Prof. Soedarto SH, Tembalang, Semarang 50275, Central Java, Indonesia² Department of Health Sciences, Faculty of Medical Sciences, Kyushu University, 3-1-1 Maidashi, Higashi-Ku, Fukuoka 812-8582, Japan³ Department of Applied Physics and Medical Imaging, California State University Channel Islands, Camarillo, CA 93012, United States of America⁴ Department of Metallurgical and Materials Engineering, University of Indonesia, Depok 16424, Indonesia⁵ Department of Chemical Engineering, University of Riau, Pekanbaru 28293, IndonesiaE-mail: herisutanto@live.undip.ac.id**Keywords:** thyroid shields, bolus, radibarrier, dose reduction, CT scan**Abstract**

This study was to evaluate dose reduction and resulting image quality of a new synthetic thyroid shield based on silicon rubber (SR)–lead (Pb) composites and compare to tungsten paper (WP) and a Radibarrier thyroid shields in CT examination of the neck. The synthetic SR-Pb thyroid shield had a Pb percentage from 0 to 5 wt% and a thickness of 0.6 cm. Scanning on the neck of an anthropomorphic phantom was performed with and without the SR-Pb, WP, and Radibarrier thyroid shields. The thyroid shields were placed directly on the neck surface. The thyroid dose was measured using radiophoto-luminescence (RPL) detectors. Image quality was characterized by consistency of the Hounsfield unit (HU) on the areas of anterior, posterior and lateral of the neck phantom. Detailed evaluation of the image quality was employed by image subtraction. It was found that the thyroid dose at the surface decreased with an increase of Pb percentage in the SR-Pb shield. The thyroid dose reduction was 34% for a Pb percentage of 5 wt%. The reduction of the dose using WP and Radibarrier were 36% and 67%, respectively. The dose reduction when using the WP and Radibarrier was higher than when using the SR-Pb 5 wt% thyroid shield. However the existence of artifact in the WP and the Radibarrier reduced the image quality, indicated by a significant change of HU, i.e. the increases of HU in the posterior area were 77% for the WP and 553% for the Radibarrier. The SR-Pb shield produced only a very small artifact, resulting in an increase of HU in the posterior area of only 9%. The SR-Pb shield is suitable in the daily clinical setting for thyroid dose reduction in CT examinations while maintaining image quality.

Introduction

Computed tomography (CT) provides excellent images for diagnosing patient abnormalities [1], however the dose received by radiosensitive organs, specifically to the superficial organs such as the thyroid, gonads, eye lens and breast, is a significant concern [2–12]. These organs are composed of radio-sensitive cells and have a greater risk of developing cancer in the future [4, 6, 10, 11, 13–17]. Among the most frequent CT examinations are head, thorax, cervical spine and neck. In these CT examinations, the thyroid glands is often exposed to the primary beam and receives high dose [6–8, 17, 18]. The International

Commission on Radiological Protection (ICRP) reported that the thyroid has a tissue weighting factor (W_T) of 0.04, meaning that the risk is very high [19, 20]. Therefore, it is crucial to reduce the dose received by the thyroid as much as possible while maintaining image quality [19, 20]. Dose optimization should be kept in mind because of the inverse relationship between good image quality and low radiation doses [4, 21–23].

A straightforward method to optimize thyroid dose and image quality in the CT examination is using a thyroid shield which is commercially available and is based on bismuth-latex [24]. Gbelcova *et al* [25] reported that the reduction of dose by a thyroid shield is in

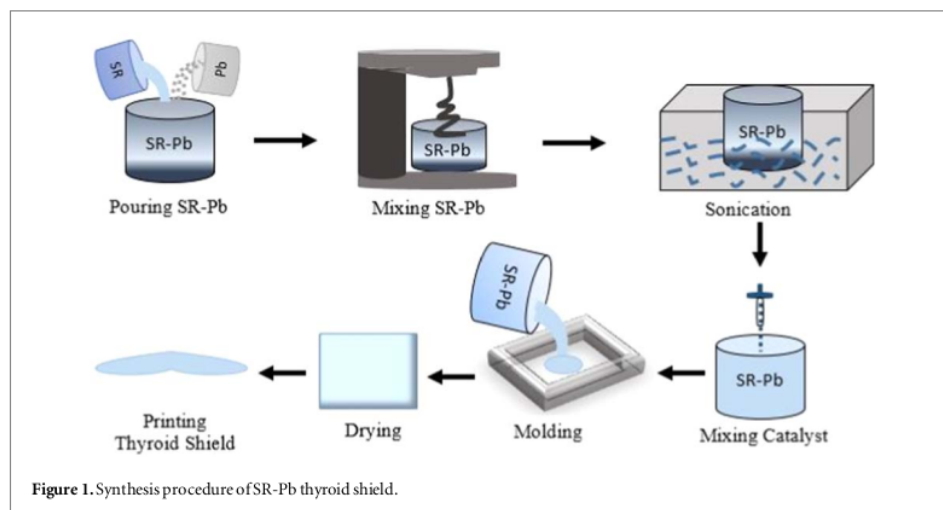


Figure 1. Synthesis procedure of SR-Pb thyroid shield.

the range from 23% to 35%. This agrees with other studies reporting thyroid dose reductions from 25 to 40% [18, 26, 27]. However, the main limitation of the bismuth shield is that it causes artifact in the image, especially in areas close to the thyroid shield, due to the x-ray transmissions that are supposed to contribute to the image which are absorbed by the material of the thyroid shield itself [10, 24, 28].

Currently, a common strategy to optimize the thyroid dose by automatic tube current modulation (ATCM) [29]. Hoang *et al* [18] reported that by using ATCM, thyroid dose decreased by up to 29.5% and there was no significant degradation of image quality. The similar results were also reported elsewhere [18, 26, 27]. A combination of ATCM and thyroid shield will further increase a dose reduction. Inkoom *et al* [28] reported that combination of both can increase the reduction of thyroid dose from 22.5% to 78%. However, many studies reported that a combination of both causes unpredictable dose result when thyroid shield is located before scanning of scout [20, 22]. The dose reduction is difficult to evaluate, because ATCM depends on the region scanned and patient body habitus and is affected by thyroid shield [21, 30–32]. Nowadays, the ATCM is commonly used in the most modern CT, however, it should be noted that not all CT scans are equipped with ATCM feature.

Correspondingly, based on these available strategies, thyroid shield remains the choice for CT scan that is not featured with ATCM or to be used as combination with ATCM. Most thyroid shields are made from Bismuth-latex, because of its high atomic number ($Z = 83$) and consequent high ability to absorb radiation [33]. To minimize the artifact of the resulting image caused by the thyroid shield, many studies recommend a spacer from 1 to 3 cm between the thyroid shield and the neck [6, 18, 34]. By adding distance, it was reported there is no significant change in HU


values with and without thyroid shield. However, an addition of a spacer may be time-consuming and prolong examination time in the clinical practice. Therefore, efforts to develop a new thyroid shield that can effectively reduce doses while minimizing or even removing the artifacts need to be considered.

Recently Irdawati *et al* [35] proposed a new material for superficial organ shield based on silicon rubber (SR) and lead (Pb). It was reported that the SR-Pb has a good ability as an eye shield with a dose reduction up to 50% without any artifact appearing in the image even though it is placed directly on the organ surface [35]. Although SR-Pb is a promising material as a superficial organ shield, it has not applied to any other organ other than the eye lens. The aim of this study, therefore, was to investigate the ability of a SR-Pb shield, placed directly on the neck surface, to reduce the dose to the thyroid during CT neck examination. We compared it to other thyroid shields such as Tungsten paper (WP) and Radibarrier.

Materials and methods

Synthesis procedure of SR-Pb shield

The thyroid shield was synthesized from silicon rubber (SR-RTV52) and lead type lead (II) acetate trihydrate ($\text{Pb}(\text{CH}_3\text{COO})_2 \cdot 3\text{H}_2\text{O}$). There were many steps to synthesis the SR-Pb shield (figure 1). The first step was pouring SR and Pb to beaker glass with different percentage of Pb from 0 to 5 wt%. Afterwards, it was then mixed for 30 min. To increase homogeneity of SR-Pb, sonication was carried out with an ultrasonic bath. The next step was the vulcanization process to accelerate the drying process of the thyroid shield. After the thyroid shield dries, it was ready to print the shield according to the shape of the neck.

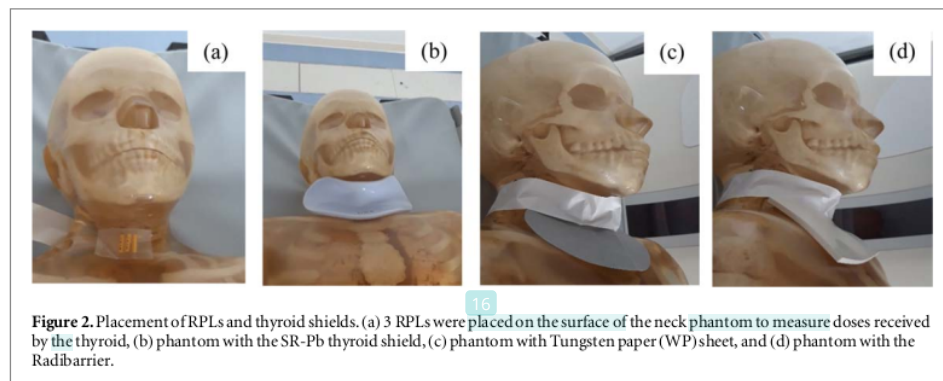

Characterization of the SR-Pb shield

There are at least two important parameters of SR-Pb as an organ shield need to be characterized. The two characteristics of SR-Pb are effective atomic number (Z_{eff}) and elasticity. The Z_{eff} is the most important parameters for tissue equivalence, radiation scattering, radiation absorption, and shielding effectiveness for x-ray radiation. The Z_{eff} of SR-Pb with different percentage of Pb from 0 to 5 wt% were calculated using Auto- Z_{eff} software version 1.7 [36]. The elasticity of the SR-Pb is also important due to its placement in irregular shape of the neck surface. For quantitative analysis, the elasticity of SR-Pb thyroid shield was measured by the value of the Young modulus and strain. The Young modulus is a measure of the stiffness of an elastic material, and the strain is the degree of change in the length of material for a given force.

Dose measurement

The dose received by thyroid with and without the SR-Pb thyroid shield was measured using Radiophotoluminescence (RPL) glass detectors type GD-352M (Chiyoda Technol Corporation, Japan). The RPL detectors had a sensitivity range from 10 μGy to 10 Gy. Three RPLs were placed on the surface of the neck anthropomorphic phantom, as shown in figure 2(a). The SR-Pb was shown in figure 2(b). The SR-Pb shield was compared with Tungsten paper (WP) (Toppan Printing and Kyoto University, Japan) (figure 2(c)) and Radibarrier (Shin Etsu Chemical, Japan) (figure 2(d)). The WP and Radibarrier have a thickness of 10 mm.

There were many steps in dose measurement using RPLs. After annealing at a temperature of 400 °C to remove the previous dose stored, the initial dose value before irradiation is read to determine the background dose. Following the irradiation process, the RPLs were pre-heated at 80 °C and read using the reader of Dose Ace type FDG-1000 (Chiyoda Technol Corporation, Japan). The scanning parameters were tabulated in table 1. Each examination was repeated three times to verify the effect of the shield in reducing organ dose.

Table 1. The scanning parameters.

Tube voltage	120 kVp
Tube current	150 mA
Time rotation	0.75 s rot^{-1}
Slice thickness	5 mm
Field of view (FOV)	320 mm
Scan type	Helical
Pitch	1.375

Image quality evaluation

The image quality with and without thyroid shield was evaluated and compared. Image quality evaluation is based on the consistency of HU values. Larger HU values compared with the image without the thyroid shield were indicative of the presence of artifact in the image. For quantitative analysis, artifact in the image was evaluated with four circular region of interests (ROIs) at areas of the anterior (i.e. at the area of the thyroid), lateral soft tissue (i.e. right and left side) and at the posterior of the neck. The size of each ROI was 112.14 mm^2 . Locations of the ROIs in the image are shown in figure 3. For a detailed evaluation of image quality, image subtraction between images using a thyroid shield and without it was performed.

Results

Characteristics of the SR-Pb shield

Figure 4 shows the Z_{eff} of the SR-Pb as a function of photon energy for various Pb percentage from 0 up to 5 wt%. The Z_{eff} values were constant in the intermediate energy region (0.5–5 MeV) and in the very high energy (>100 MeV). A variation was observed in the lower energy (0.01–0.1 MeV) and in the high energy regions (5–100 MeV). It is found that the Z_{eff} values increased with an increase in Pb content in the SR-Pb as predicted.

Figure 5 shows that the addition of Pb percentage caused an increase of Young modulus and a decrease of strain value. This happens because the level of deformation of the chain of SR molecules is limited by Pb and leads to increased stiffness and decreased

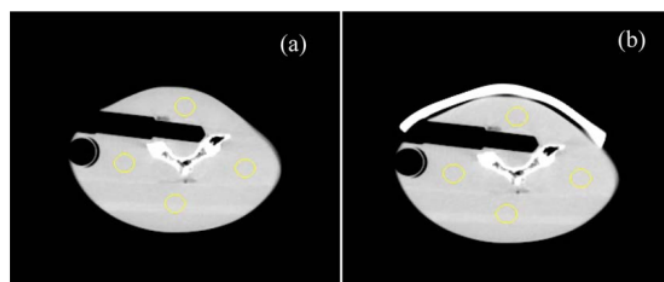


Figure 3. Locations of the ROIs to calculate HU values. (a) Without thyroid shield, and (b) With SR-Pb thyroid shield.

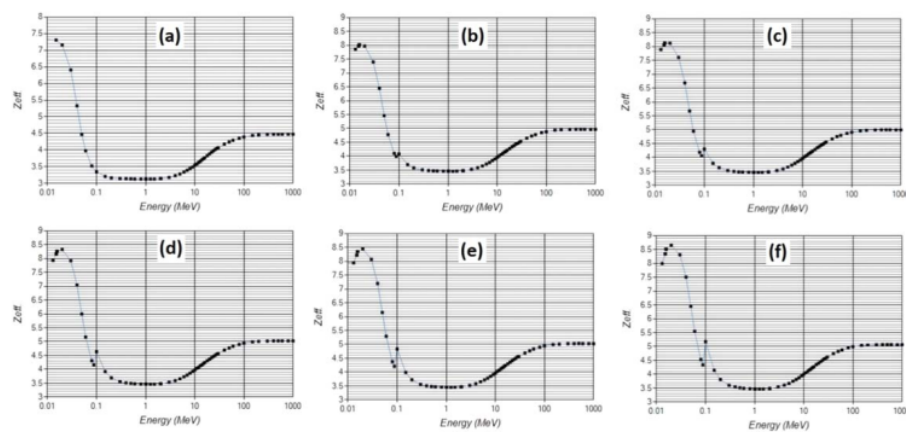


Figure 4. The Z_{eff} of the SR-Pb as a function of photon energy for various Pb percentage. (a) SR-Pb 0 wt%, (b) SR-Pb 1 wt%, (c) SR-Pb 2 wt%, (d) SR-Pb 3 wt%, (e) SR-Pb 4 wt%, and (f) SR-Pb 5 wt%.

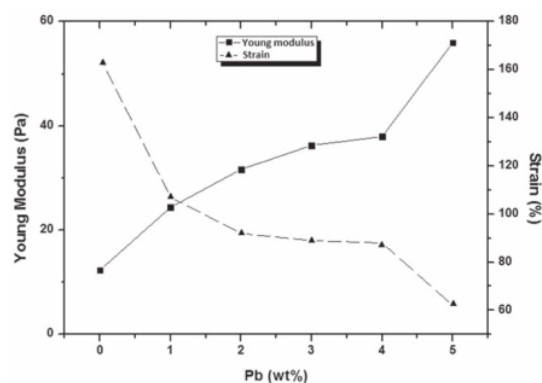


Figure 5. Yong modulus and strain of the SR-Pb thyroid shield for various Pb percentage from 0 up to 5 wt%.

change in the length of a material [37–39]. The thyroid shield with Pb 5 wt% has a value of the Young modulus and strain of 55.96 Pa and 62%, respectively. These values indicate that it still has sufficient elasticity to cover a non-flat organ such as the neck surface.

Figure 2(b) shows visually the elasticity of the SR-Pb thyroid shields so that its placement in the throid area is very easy. This differs from Tungsten paper (WP) (figure 2(c)) and the Radibarrier (figure 2(d)), which

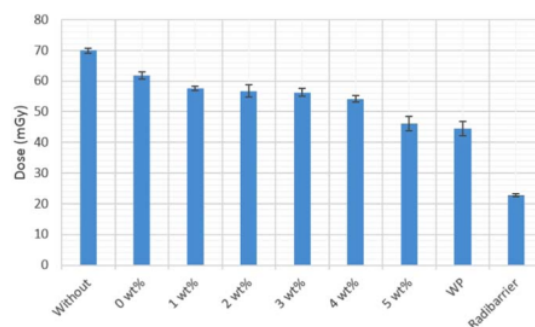


Figure 6. Thyroid dose in the CT examination of the neck, with and without thyroid shields.

do not have good elasticity and require tape to locate them in position on the thyroid area.

Effect of thyroid shields on the dose reduction

The superficial dose at the thyroid during CT examination of the neck using SR-Pb thyroid shields with a Pb content from 0 to 5 wt%, and its comparison with the WP and the Radibarrier thyroid shields, can be seen in figure 6. The dose without thyroid shield 69.855 ± 0.8 mGy, and the dose reductions with the SR-Pb thyroid shields with variation of Pb percentage of 0, 1, 2, 3, 4 and 5 wt% are 12%, 18%, 19%, 20%, 22% and 34%, respectively. It also shows that the Radibarrier has the greatest ability to reduce the dose to the thyroid, compared with SR-Pb and WP thyroid shields.

Effect of thyroid shield on the image quality

Neck images with and without thyroid shields are shown in figure 7. The resulting images using the SR-Pb thyroid shield do not reveal any artifacts in the thyroid (anterior area), lateral areas and posterior area, while the WP shield causes significant artifact in the anterior area, and minor artifact in the lateral and posterior areas. The Radibarrier provides severe artifact in all areas of the image (anterior, posterior and lateral).

The artifacts in the resulting image can be identified by increased HU values and its standard deviations in the anterior, lateral and posterior regions, tabulated in table 2. The HU values of the SR-Pb increased slightly compared to those without the thyroid shield (8.8%), while the HU values in the anterior (thyroid area) of the WP and the Radibarrier increase significantly by up to 77.0% and 552.7%, respectively. Image quality using the SR-Pb shield was maintained, as evidenced by the SD values being similar to without the thyroid shield. WP and Radibarrier have higher difference SD values when compared with the image without a shield.

To ensure that the SR-Pb thyroid shield does not cause artifact in the resulting image, a detailed

evaluation using subtraction image between the image with and without thyroid shield was conducted. The subtraction images are shown in figure 8. This shows that using the SR-Pb with various percentages of Pb from 0–5 wt%, the resulting image can be maintained for diagnostic purposes because there is only a small artifact. Conversely, WP and the Radibarrier cannot be used for diagnostic purposes because both cause severe artifact in the image.

Discussion

One straightforward method to reduce the surface dose on CT examination, including the dose on the surface of the thyroid, is to use an organ shield. The main problem with the use of organ shields is the appearance of artifacts in the image that can interfere with diagnosis [24–28]. In the hope of avoiding artifact, a previous study developed a new material for an organ shield from SR material mixed with variation percentages of Pb from 0 to 5 wt% [35]. Increasing the Pb content leads to an increase in the dose reduction of the surface of eye lens. The addition of Pb 5 wt% in the SR-Pb shield can reduce the eye dose up to 50% [35]. Dose reduction in the thyroid (34%) is smaller than in the eye lens likely because the SR-Pb shield protects from many sides (i.e. above, right and left sides), while in the thyroid, the SR-Pb shield protects radiation only from above. A better design of the thyroid shield may be able increase dose reduction.

The use of a SR-Pb shield has only a slight impact on the resulting image. The quality of the image is maintained for diagnostic proposes, even though the SR-Pb thyroid shield is in contact with the surface of the organ, i.e. thyroid or eye lens.

The WP and Radibarrier shields reduce thyroid dose by more than the SR-Pb shield, viz. 36% and 67%, respectively. However the resulting images suffer severe artifacts which can lead to mis-diagnosis in the anterior, posterior and lateral areas. Radiation absorption depends on the atomic number (Z) of material, with higher atomic number material having a greater

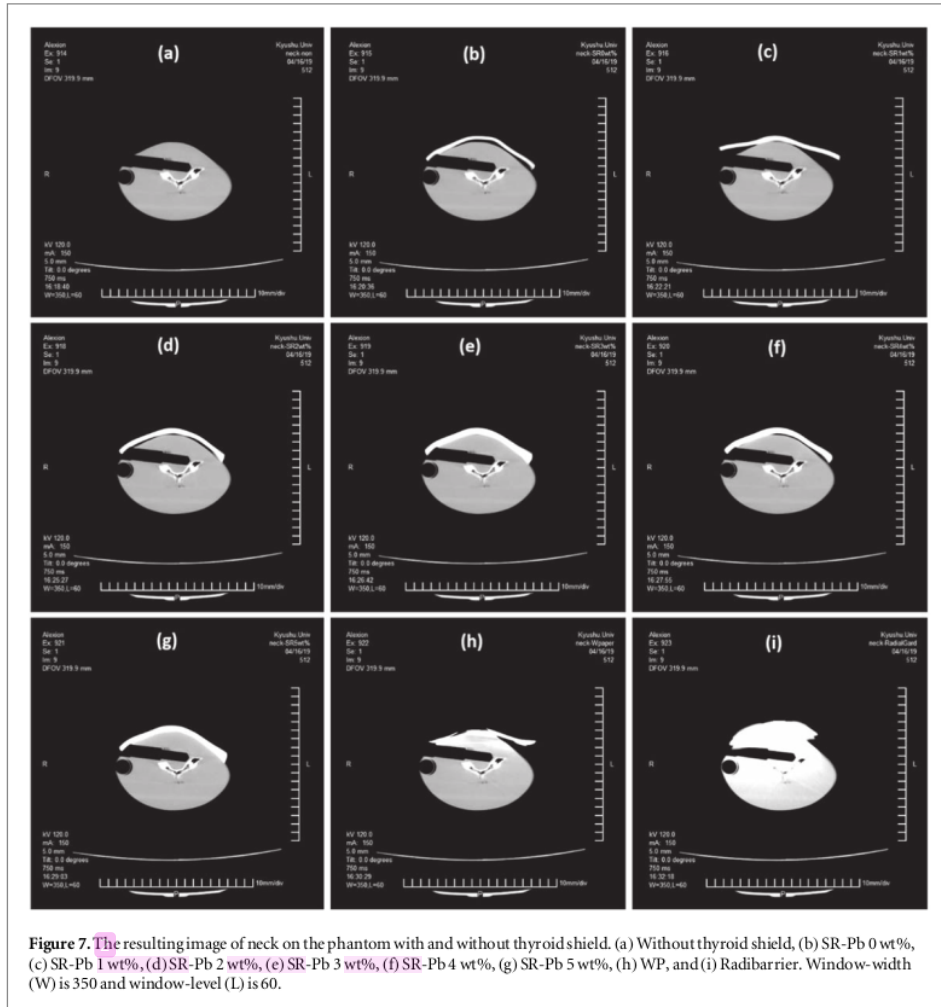


Figure 7. The resulting image of neck on the phantom with and without thyroid shield. (a) Without thyroid shield, (b) SR-Pb 0 wt%, (c) SR-Pb 1 wt%, (d) SR-Pb 2 wt%, (e) SR-Pb 3 wt%, (f) SR-Pb 4 wt%, (g) SR-Pb 5 wt%, (h) WP, and (i) Radibarrier. Window-width (W) is 350 and window-level (L) is 60.

Table 2. HU values and standard deviation of various thyroid shields in four ROI locations.

Thyroid shield	Area (mm ²)	Lateral							
		Anterior		Right side				Posterior	
		HU	SD	HU	SD	HU	SD	HU	SD
Without	112.14	119.25	2.41	125.30	2.19	125.30	2.29	126.39	3.62
SR-Pb 0 wt%	112.14	120.04	2.60	126.26	1.88	119.16	2.59	126.51	4.03
SR-Pb 1 wt%	112.14	125.37	2.83	121.21	2.27	123.74	2.37	126.73	4.35
SR-Pb 2 wt%	112.14	123.73	3.12	127.71	2.07	120.97	2.85	126.25	3.91
SR-Pb 3 wt%	112.14	126.69	3.32	128.98	2.45	120.67	2.69	127.59	3.87
SR-Pb 4 wt%	112.14	128.84	3.20	129.15	2.30	120.71	2.64	127.71	3.60
SR-Pb 5 wt%	112.14	129.78	4.17	128.62	2.33	122.58	2.69	127.74	3.95
WP	112.14	211.05	19.42	143.98	3.09	133.34	3.39	135.30	3.64
Radibarrier	112.14	778.39	148.69	215.36	8.29	296.51	18.15	202.38	6.67

ability to absorb radiation [33, 40]. Tungsten (W) has a Z value of 71 and its percentage in the WP shield is about 80%, while the Radibarrier has a lead equivalent of 1.1 mm, where lead has a Z value of 82.

Unfortunately both cause significant artifacts and noise in the resulting image. In the SR-Pb shield, the Pb content is low (0–5 wt%) so that the Pb is

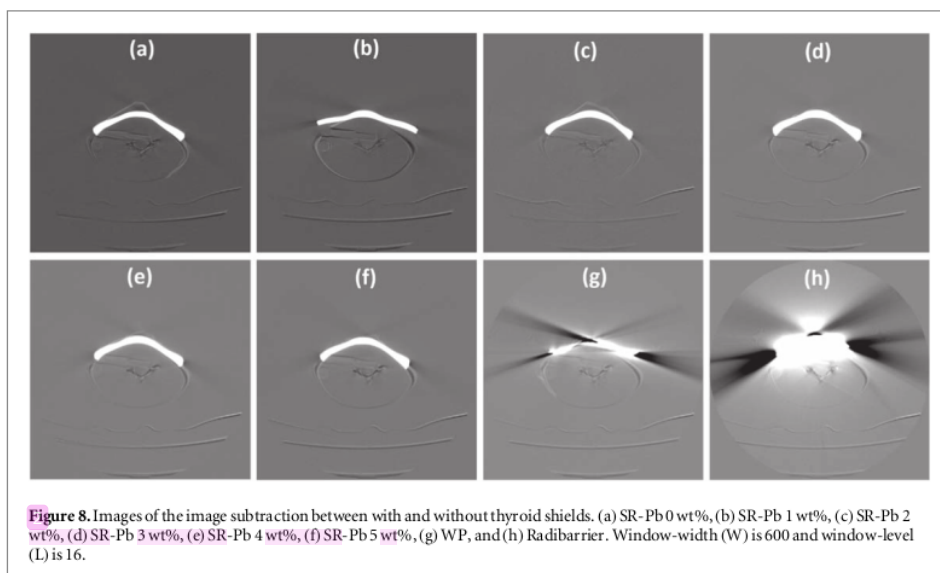


Figure 8. Images of the image subtraction between with and without thyroid shields. (a) SR-Pb 0 wt%, (b) SR-Pb 1 wt%, (c) SR-Pb 2 wt%, (d) SR-Pb 3 wt%, (e) SR-Pb 4 wt%, (f) SR-Pb 5 wt%, (g) WP, and (h) RadibARRIER. Window-width (W) is 600 and window-level (L) is 16.

distributed uniformly in the SR-Pb sheet, hence artifact can be avoided.

The protection of thyroid gland is crucial because the thyroid is one of the most radiosensitive organs and is vulnerable to stochastic effects such as cancer. Based on our results, the SR-Pb thyroid shield may be recommended in the CT examination of the neck replacing the bismuth thyroid shield. Even though the reduction dose of SR-Pb is smaller than bismuth shield, it is preferred because artifact is almost non-existent in the SR-Pb.

The SR-Pb thyroid shield is non-toxic, so it is safe to use. Another advantage is its elasticity, so it is easy to use, easily positioned and removed, and has sufficient flexibility to cover an organ. It is not time-consuming to use, and therefore dose reduction does not prolong examination time. It is light-weight so that patients will feel comfortable when using it. It may also reduce the patient's anxiety about the impact of radiation, because the patient is aware that he/she is protected.

The limitations of this study are that validation was only performed on a phantom, with a single size representing an average-size patient not pediatric or obese patient, and the image quality was evaluated quantitatively without observation by expert radiologists. A further study on SR-Pb thyroid shield with a possible combination of the ATCM might be more challenging. In the CT examination equipped with ATCM, the SR-Pb placement before the scout might change the current in the ATCM, so that in clinical applications, SR-Pb should be placed after scout image is obtained.

Conclusions

The thyroid shield made from SR-Pb has been successfully synthesized and validated. The use of the SR-Pb thyroid shield can reduce thyroid dose. The reduction in dose increases with the increasing percentage of Pb. In SR-Pb 5 wt% the decreasing in dose was 34% compared with having no thyroid shield. The resulting image is of high quality without artifact even at higher percentage of Pb so that it can be used without mis-diagnosis. The SR-Pb thyroid shield is very practical because it can be placed directly above the surface of the thyroid, and is sufficiently flexible to cover the thyroid. Hence, we recommend its adoption for clinical CT neck examinations.

Acknowledgments

The authors would like to thank the Ministry of research, Technology and Higher Education of the Republic of Indonesia for funding this research in 2019.

ORCID iDs

Heri Sutanto <https://orcid.org/0000-0001-7119-9633>

Choirul Anam <https://orcid.org/0000-0003-0156-6797>

Eko Hidayanto <https://orcid.org/0000-0002-3438-0369>

References

- [1] Anam C, Fujibuchi T, Budi W S, Haryanto F and Dougherty G 2018 An algorithm for automated modulation transfer

- function measurement using an edge of a PMMA phantom: Impact of field of view on spatial resolution of CT images *J. Appl. Clin. Med. Phys.* **19** 244–52
- [2] Lewis M A and Edyvean S 2005 Patient dose reduction in CT *Br. J. Radiol.* **78** 880–3
- [3] Geleijns J, Salvadó Artells M, Veldkamp W J, López Tortosa M and Calzado Cantera A 2006 Quantitative assessment of selective in-plane shielding of tissues in computed tomography through evaluation of absorbed dose and image quality *Eur. J. Radiol.* **16** 2334–40
- [4] Brenner D J and Halle J 2007 Computed tomography—an increasing source of radiation exposure *N. Engl. J. Med.* **357** 2277–84
- [5] Goldman L W 2007 Principles of CT: radiation dose and image quality *Nucl. Med. Technol.* **35** 213–25
- [6] Catuzzo P *et al* 2010 Dose reduction in multislice CT by means of bismuth shields: results of *in vivo* measurements and computed evaluation *Radiol. Med.* **115** 152–69
- [7] Gunn M L, Kanal K M, Kolokythas O and Anzai Y 2009 Radiation dose to the thyroid gland and breast from multidetector computed tomography of the cervical spine: does bismuth shielding with and without a cervical collar reduce dose? *J. Comput. Assist. Tomogr.* **33** 987–90
- [8] Chang K H, Lee W, Choo D M, Lee C S and Kim Y 2009 Dose reduction in CT using bismuth shielding: measurements and Monte Carlo simulations *Radiat. Prot. Dosimetry* **138** 382–8
- [9] Brenner A D J 2010 Slowing the increase in the population dose resulting from CT scans slowing the increase in the population dose resulting from CT scans *Radiat. Res. Soc.* **174** 809–15
- [10] Antypas E J *et al* 2011 A comprehensive approach to CT radiation dose reduction: one institution's experience *Am. J. Roentgenol.* **197** 935–40
- [11] Alkhorayef M, Babikir E, Alrushoud A, Al-mohammed H and Sulieman A 2017 Patient radiation biological risk in computed tomography angiography procedure *Saudi J. Biol. Sci.* **24** 235–40
- [12] Alkhorayef M, Sulieman M, Alonazi B, Alnaaimi M, Alduaij M and Bradley D 2019 Estimation of radiation-induced cataract and cancer risks during routine CT head procedures *Radiat. Phys. Chem.* **155** 65–8
- [13] Kim K P *et al* 2012 Development of a database of organ doses for paediatric and young adult CT scans in the United Kingdom *Radiat. Prot. Dosimetry* **150** 415–26
- [14] Hamada N and Fujimichi Y 2014 Classification of radiation effects for dose limitation purposes: history, current situation and future prospects *Radiat. Res.* **55** 629–40
- [15] Chen J X, Kachniarz B, Gilani S and Shin J J 2013 Risk of malignancy associated with head and neck CT in children: a systematic review *Otolaryngol. Head. Neck. Surg.* **151** 554–66
- [16] Akhlaghi P, Hakimabad H M and Motavalli L R 2013 An overview of exposure parameters, dose measurements and strategies for dose reduction in pediatric CT examinations *Radioprotection* **49** 9–15
- [17] Alonso T C, Mourão A P, Santana P C and Teógenes A 2016 Assessment of breast absorbed doses during thoracic computed tomography scan to evaluate the effectiveness of bismuth shielding *Appl. Radiat. Isot.* **117** 55–7
- [18] Hoang J K *et al* 2012 Organ-based dose current modulation and thyroid shields: techniques of radiation dose reduction for neck CT *Am. J. Roentgenol.* **198** 1132–8
- [19] Mendes M, Costa F, Figueira C, Madeira P, Teles P and Vaz P 2015 Assessment of patient dose reduction by Bismuth shielding in CT using measurements, GEANT4 and MCNPX simulations *Radiat. Prot. Dosimetry* **165** 175–81
- [20] Lawrence S and Seeram E 2017 The current use and effectiveness of bismuth shielding in computed tomography: a systematic review *Radiol. Open. J.* **2** 7–16
- [21] Russell M T, Fink J R, Rebeles F, Kanal K and Ramos M 2008 Balancing radiation dose and image quality: clinical applications of neck volume CT *Am. J. Neuroradiol.* **29** 727–31
- [22] Samei E 2014 Pros and cons of organ shielding for CT imaging *Pediatr. Radiol.* **44** 495–500
- [23] Anam C *et al* 2019 Assessment of patient dose and noise level of clinical CT images: automated measurements *J. Radiol. Prot.* **39** 783–93
- [24] Hohl C *et al* 2009 Radiation dose reduction to breast and thyroid during MDCT: effectiveness of an in-plane bismuth shield *Acta. Radiol.* **47** 562–7
- [25] Gbelcová L, Nikodemová D and Horváthová M 2011 Dose reduction using bismuth shielding during paediatric CT examinations in Slovakia *Radiat. Prot. Dosimetry* **147** 160–3
- [26] Nikodemova D and Horva M 2011 Dose reduction using bismuth shielding during paediatric CT examinations in slovakia *Radiat. Prot. Dosimetry* **147** 160–3
- [27] Lee Y H *et al* 2011 Comparative analysis of radiation dose and image quality between thyroid shielding and unshielding during CT examination of the neck *Am. J. Roentgenol.* **196** 611–5
- [28] Inkoom S *et al* 2017 Paediatric neck multidetector computed tomography: the effect of bismuth shielding on thyroid dose and image quality *Radiat. Prot. Dosimetry* **173** 361–73
- [29] Anam C, Haryanto F, Widita R, Arif I, Dougherty G and McLean D 2018 Volume computed tomography dose index (CTDIvol) and size-specific dose estimate (SSDE) for tube current modulation (TCM) in CT scanning *Int. J. Radiat. Res.* **16** 289–97
- [30] Solomon J B, Li X and Samei E 2013 Relating noise to image quality indicators in CT examinations with tube current modulation *Am. J. Roentgenol.* **200** 592–600
- [31] Papadakis A E, Perisinakis K and Damilakis J 2014 Automatic exposure control in CT: the effect of patient size, anatomical region and prescribed modulation strength on tube current and image quality *Eur. J. Radiol.* **24** 2520–31
- [32] Leswick D A, Hunt M M, Webster S T and Fladeland D A 2008 Thyroid shields versus z-axis automatic tube current modulation for dose reduction at neck CT *Radiology* **249** 572–80
- [33] La L B T *et al* 2016 X-ray protection, surface chemistry and rheology of ball-milled submicron Gd₂O₃ aqueous suspension *Colloids Surf. A* **501** 75–82
- [34] Zhang J and Oates M E 2012 CT bismuth breast shielding: Is it time to make your own decision? *J. Am. Coll. Radiol.* **9** 856–8
- [35] Irdawati Y, Sutanto H, Anam C, Fujibuchi T, Zahroh F and Dougherty G 2019 Development of a novel artifact-free eye shield based on silicon rubber-lead composition in the CT examination on the head *J. Radiol. Prot.* **39** 991–1005
- [36] Taylor M L, Smith R L, Dossing F and Franich R D 2012 Robust calculation of effective atomic numbers: the Auto-Zeff software *Med. Phys.* **39** 1769–78
- [37] Araby S, Zhang L, Kuan H C, Dai J B, Majewski P and Ma J 2013 A novel approach to electrically and thermally conductive elastomers using graphene *Polymer* **54** 3663–70
- [38] Kang H, Zuo K, Wang Z, Zhang L, Liu L and Guo B 2014 Using a green method to develop graphene oxide/elastomers nanocomposites with combination of high barrier and mechanical performance *Compos. Sci. Technol.* **92** 1–8
- [39] Yang H *et al* 2018 Highly sensitive and stretchable graphene-silicone rubber composites for strain sensing *Compos. Sci. Technol.* **167** 371–8
- [40] Atashi P, Rahmani S, Ahadi B and Rahmati A 2018 Efficient, flexible and lead-free composite based on room temperature vulcanizing silicone rubber/W/Bi₂O₃ for gamma ray shielding application *J. Mater. Sci., Mater. Electron.* **29** 12306–22

10. An artifact-free thyroid shield in CT examination a phantom study

ORIGINALITY REPORT

10%

SIMILARITY INDEX

5%

INTERNET SOURCES

8%

PUBLICATIONS

2%

STUDENT PAPERS

PRIMARY SOURCES

- | | | |
|---|---|------|
| 1 | G Díaz Londoño, S García-Pareja, F Salvat, A M Lallena. "Simple variance reduction in Monte Carlo calculations of specific absorbed fractions: Russian roulette and splitting at the source organ", Biomedical Physics & Engineering Express, 2020
Publication | 1 % |
| 2 | Bratati Pradhan. "Preparation and characterization of exfoliated layered double hydroxide/silicone rubber nanocomposites", Journal of Applied Polymer Science, 01/05/2011
Publication | 1 % |
| 3 | Submitted to Universitas Diponegoro
Student Paper | 1 % |
| 4 | IFMBE Proceedings, 2009.
Publication | 1 % |
| 5 | P. Catuzzo. "Dose reduction in multislice CT by means of bismuth shields: results of in vivo | <1 % |

measurements and computed evaluation", La radiologia medica, 12/14/2009

Publication

6	www.ncbi.nlm.nih.gov Internet Source	<1 %
7	boristheses.unibe.ch Internet Source	<1 %
8	link.springer.com Internet Source	<1 %
9	C. Hohl. "Radiation Dose Reduction to Breast and Thyroid During MDCT: Effectiveness of an In - Plane Bismuth Shield", Acta Radiologica, 6/1/2006 Publication	<1 %
10	V. P. Singh, N.M. Badiger, N. Kucuk. "Assessment of methods for estimation of effective atomic numbers of common human organ and tissue substitutes: waxes, plastics and polymers", Radioprotection, 2014 Publication	<1 %
11	Submitted to Cardiff University Student Paper	<1 %
12	Parinaz Mehnati, Reza Malekzadeh, Mohammad Yousefi Sooteh, Soheila Refahi. "Assessment of the efficiency of new bismuth composite shields in radiation dose decline to	<1 %

13

D. E. Heaney. "A Comparison of reduction in
CT dose through the use of gantry
angulations or bismuth shields", Australasian
Physics & Engineering Sciences in Medicine,
06/2006

Publication

<1 %

14

openventio.org

Internet Source

<1 %

15

"Trends in Mechanical and Biomedical
Design", Springer Science and Business Media
LLC, 2021

Publication

<1 %

16

AD Goren, RD Prins, LT Dauer, B Quinn, A Al-
Najjar, RD Faber, G Patchell, I Branets, DC
Colosi. "Effect of leaded glasses and thyroid
shielding on cone beam CT radiation dose in
an adult female phantom", Dentomaxillofacial
Radiology, 2013

Publication

<1 %

17

Martin L. Gunn. "Radiation Dose to the
Thyroid Gland and Breast From Multidetector
Computed Tomography of the Cervical Spine :
Does Bismuth Shielding With and Without a
Cervical Collar Reduce Dose?", Journal of
Computer Assisted Tomography, 11/2009

<1 %

18

fbt.tums.ac.ir

Internet Source

<1 %

19

library.unisel.edu.my

Internet Source

<1 %

20

www.ajronline.org

Internet Source

<1 %

21

"Highlights of articles in this issue", Journal of Radiological Protection, 2019

Publication

<1 %

22

"Pediatric Oculoplastic Surgery", Springer Science and Business Media LLC, 2018

Publication

<1 %

23

Abdelmoneim Sulieman, Kholoud S. Almogren, Nissren Tamam. "Radiation exposure estimation in pediatric patients during computed tomography imaging procedures", Radiation Physics and Chemistry, 2023

Publication

<1 %

24

businessdocbox.com

Internet Source

<1 %

25

open.uct.ac.za

Internet Source

<1 %

26

usir.salford.ac.uk

Internet Source

<1 %

27

Medical Radiology, 2012.

Publication

<1 %

28

A Hidalgo, J Davies, K Horner, C Theodorakou.
"Effectiveness of thyroid gland shielding in
dental CBCT using a paediatric
anthropomorphic phantom",
Dentomaxillofacial Radiology, 2015

Publication

<1 %

Exclude quotes Off

Exclude matches Off

Exclude bibliography On