

HiroshimaJMedSci_67s_161.pdf

by

Submission date: 15-Jul-2020 01:28PM (UTC+0700)

Submission ID: 1357733367

File name: HiroshimaJMedSci_67s_161.pdf (212.19K)

Word count: 2612

Character count: 14068

Effects of Neo Automatic Code on the Accuracy of Chest Compression Depths in Cardiac Arrest Patients

Rendi Editya DARMAWAN¹⁾, Untung SUJIANTO²⁾, Nana ROCHANA^{2) *}

¹ Master Program in Nursing, Faculty of Medicine, Diponegoro University, Indonesia

² Department of Nursing, Faculty of Medicine, Diponegoro University, Indonesia

ABSTRACT

Objective: to analyze the effects of manual chest compression using neo automatic code on the accuracy of compression depths. Methods: This study used a quantitative, post test quasi-experimental design with a control group. The samples were 74 cardiac arrest patients in two hospitals in Surakarta and Klaten, who were selected using purposive sampling technique. The data were analyzed by the Mann-Whitney test. Results: the mean of accuracy of compression depth in the control group was $68.10 \pm 17.60\%$, and in the treatment group was $83 \pm 6.04\%$. The result of statistical analysis showed that there were differences in the accuracy of compression depth in the intervention and control group with p-value of 0.000. Conclusion: there were effects of manual chest compression using neo automatic code on the accuracy of compression depths. Neo automatic code could improve the accuracy of chest compression depths.

Keywords: cardiac arrest, chest compression, compression depth accuracy, neo automatic

The burden of cardiac arrest in health sectors is substantial with an estimated 424,000 and 275,000 cardiac arrests occurring each year in the USA and in Europe respectively. Moreover, a number of patients who survived cardiac arrest in North America and the UK in 2016 were less than 10% ⁽¹⁾. However, the incident of cardiac arrest in Indonesia has not been reported though the prevalence of cardiac diseases and cerebrovascular accidents in 2013 were reported high of 3,180,408 and 2,137,941 respectively. These high numbers would potentially result in high incidents of cardiac arrest ⁽²⁾. Therefore, timely and high quality cardiopulmonary resuscitations (CPRs) are needed to increase cardiac arrest survivors.

Following the highlights of the 2015 American Heart Association (AHA) guidelines update for CPR, it recommends rescuers to compress the chest of adult cardiac arrest victims at 100 to 120 compressions per minute with the depth of 5 to 6 cm, to allow full chest wall recoil, and to minimize interruptions of chest compressions ⁽³⁾. Professional rescuers, however, often do not deliver high quality CPRs regarding compression rates and depths ⁽⁴⁻⁸⁾. Avoiding excessive compression rates may lead to more compressions of sufficient depths ⁽⁶⁾. This problem can be solved using metronome ⁽⁹⁾.

The metronome is a tool to guide the CPR providers in keeping an accurate chest

compression rates ⁽⁹⁾. A higher rates of recommended chest compression is needed for metronome-guided CPRs to obtain high quality chest compressions ⁽¹⁰⁾. The new generation of metronome is The Neo Automatic Code.

Neo Automatic Code is an android based application tool to control CPR chest compressions at the rates of 100 rates per minute. It has two guiding modes of CPR which are standard CPR and compression-only CPR. Moreover, it allows the rescuers to give rescue breaths and to check pulses without interrupting compressions. Neo automatic code enables the rescuers to control their breathings as they do not need to count the compressions, and to prevent them from being exhausted. Therefore, recommended chest compression depths may highly be obtained ⁽¹¹⁾. A preliminary study of Neo Automatic Code-guiding CPRs in a mannequin showed that Neo Automatic Code produced 2253 (86.70%) recommended chest compressions out of 2598 compressions ⁽¹²⁾. However, there is still no evidence regarding the effect of Neo Automatic Code on the cardiac arrest patients. This study, thereby, aimed to analyze the effect of manual chest compression using Neo Automatic Code on the accuracy of compression depths. Our hypothesis was that there were effects of manual chest compression using Neo Automatic Code on the accuracy of compression depths.

*Corresponding author : Nana Rochana; Department of Nursing, Faculty of Medicine, Diponegoro University, Jalan Prof. H. Soedarto, SH, Tembalang, Semarang, Indonesia ; (024) 76480919; Email : na2rochana@gmail.com

2

METHODS

This study used a quantitative, post test quasi-experimental design with a control group. The sample size was counted according to the previous studies was idris et al⁽⁵⁾ resulting in 74 cardiac arrest patients. The respondents were divided into treatment and control groups who were selected using purposive sampling techniques in two hospitals in Surakarta and Klaten from May to June 2017. Inclusion criteria for the samples were that patients were resuscitated on a solid surface, patients were attached with bed site

Ethics

11

This study obtained an ethical clearance from The Health Research Ethics Committee of Faculty of Medicine, University of Diponegoro with ethical clearance number of 176 / EC / FK-RSDK / IV / 2017. This study also granted permissions to undertake research from two hospitals in Surakarta and Klaten. Research ethic principles were maintained during the study by giving informed consents to the patient's families, delivering standard CPRs as AHA guideline to the treatment and control groups, using initials for respondents, keeping respondent's personal details confidential, no coercion to participate in the study, and using certified emergency practitioners as the CPR providers to minimize the harm.

RESULTS

2 by group as can be seen from table 1. The result showed that the majority of respondents in intervention and control group were 41-60 years and female. The most common rhythm in intervention and control group shortly before cardiac arrest was unshockable rhythm which were 37 respondents (100%) and 32 respondents (86%) respectively. The leading cause of cardiac arrest patients in intervention group was non cardiac (n=32, 86%) followed by cardiac (n=5, 14%) and in control group was non cardiac (n=29, 79%) followed by cardiac (n=8, 21%).

The result showed (table 2) that intervention group had on median of accuracy of compression depth was $85\% \pm \text{IQR } 77.5$ and control group was $72\% \pm \text{IQR } 10.5$. Figure 1 showed means of accuracy of compression depth in intervention 10 up was $83\% \pm 6.04$ and means of accuracy of compression depth in intervention group was $68\% \pm 17.60\%$. The range of chest compression depth accuracy in the treatment group were 70-92% while the accuracy in the control group ranged 29-96%. This meant that the treatment group had all fraction of accuracy above 60% compared to the control group which half of them were below 60%.

monitors, chest compressions was done by certified emergency nurses or certified emergency/anaesthesiology physicians with more than 20 of body mass index (BMI). Exclusion criteria for analysis were do-not-resuscitate cardiac arrest patients. The treatment group was given Neo-Automatic-Code guiding chest compressions while the control group was given standard chest compressions. The accuracy of chest compression depths was measured from the number of R waves with the height more than 10mV.

Statistics

For every compression, the bed site monitors automatically showed R wave. 20 Researchers recorded the number of R waves and the number of chest compressions performed using hand counters. The accuracy of compression depths was measured by the percentage of the number of R waves with the height more than 10 mV on the bed side monitor with the total chest compression performed. Data on age, sex of the patient, presenting heart rhythm and the main illness were extracted from medical records. The data were analyzed by the Mann-Whitney test.

The total 74 cases met the inclusion criteria, and complete data. Demographic characteristics for the study population were stratified.

The result of statistical analysis showed p value of 0.000 meaning that there were differences in the accuracy of compression depths in the intervention and control group ($p\text{-value} < 0.05$). There was a significant effect of manual chest compression using neo automatic code on the accuracy of compression depth.

DISCUSSION

The study showed that, during hospital resuscitation by professional rescuers, the accuracy of compression depth was 29-96%. The means and standard deviation of accuracy of compression depth in intervention group $83\% \pm 6.04$ greater than control group $68\% \pm 17.60\%$. The accuracy of compression depths in the intervention group which used Neo Automatic Code was far higher than the control group. Neo Automatic Code allows the rescuers to deliver compression rates constantly at 100x/min, so that appropriate compression depths could be achieved. Rescuers only follow codes for compressions, so that did not need count and makes a sound. Rescuers can breathe freely, so

that did not easily tired and make optimal compression depths ⁽¹¹⁾.

On the other hand control the group did not use neo automatic code. An absence speed regulator controlling compression rates yields chest compression faster than using neo automatic code. An increase of chest compression rates causes fatigue among the rescuers, which consequently decrease the accuracy of compression depth ^(4-6,13,14).

Field et al ⁽¹⁴⁾ show that faster compressions lead to reduced compression depths. Monsieurs et al ⁽⁶⁾ state that high compression rates are common and can be caused by stress or by the inability of rescuers to assess and control the compression rate. Very low compression rates were uncommon and may be associated with specific activities potentially interrupting chest compressions such as aspiration, intubation and defibrillation ⁽⁶⁾.

Other than compression rates, accuracy of chest compression depth ⁽¹²⁾ related to the physical fitness of the rescuer. The weight of the rescuer is an important factor in the compression depth (4). Perkins et al ⁽¹⁵⁾ find that bed height affects maximal compression forces, and makes effects on accuracy of compression depth. Jantti et al ⁽¹⁶⁾ showed the surface under the patient may affect the cardiopulmonary resuscitation (CPR) quality. The result of statistical analysis showed that there were differences in the accuracy of compression depth in the intervention and control group (p-value<0.05). This is due an absence of speed regulator to control compression rates resulting in differences in the accuracy of compression depth.

Limitations of this study was that core diseases in this study were heterogen.

Table 1. Demographicss and study characteristics stratified by group

Characteristics	Intervention group	Control group
Age		
18-40 years	5 (14 %)	6 (16 %)
41-60 years	19 (51%)	17 (46 %)
>60 years	13 (35 %)	14 (38 %)
Gender		
Male	11 (30 %)	17 (46 %)
Female	26 (70 %)	20 (54 %)
Heath rhythm		
Shockable	0 (0%)	5 (14 %)
Unshockable	37 (100%)	32 (86%)
Main illness		
Cardiact	5 (14 %)	8 (21 %)
Non Cardiact	32 (86 %)	29 (79 %)

Table 2. Accuracy of compression depth stratified by group

Group	Median (Q2)	Q1	Q3
Intervention	85,00%	77,50%	87,50%
Control	72,00%	53,50%	81,00%

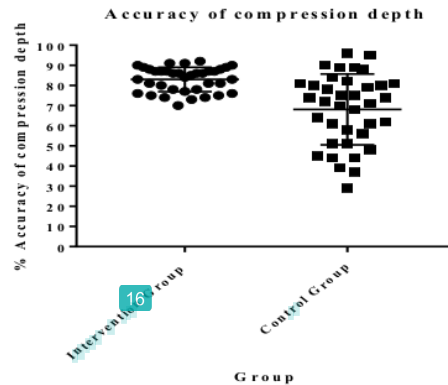


Figure 1 Accuracy of compression depth

CONCLUSIONS

There were effects of manual chest compression using neo automatic code on the accuracy of compression depth. Neo automatic code could improve the accuracy of chest compression depth. Rescuer of cardiac arrest patient must have knowledge about factors that can be improve chest compressions depth such as weight of rescuer, hard board, and chest compressions rate.

ACKNOWLEDGEMENTS

Acknowledgment of the author to the clinic thesis team and lecturers of University of Diponegoro who have motivated and provided solutive direction for us. Thanks to Ns Rakhma Anindhita, S. Kep, who helped produce chest compression codes, as well as an informatics team that has helped create neo automatic code applications. The code blue team of hospitals in Surakarta and Klaten, as well as the parties who helped smooth the research.

REFERENCES

1. Perkins GD, Lall R, Quinn T, Deakin CD, Cooke MW, Horton J, et al. Mechanical versus manual chest compression for out-of-hospital cardiac arrest (PARAMEDIC): a pragmatic, cluster randomised controlled trial. *Lancet* (London, England) [Internet]. 2015 Mar 14 [cited 2016 Sep 25];385(9972):947–55. Available from: <http://www.ncbi.nlm.nih.gov/pubmed/25467566>
2. Kementerian Kesehatan Republik Indonesia. Riset kesehatan dasar. Kemenkes RI. 2013;
3. AHA. Highlights of the 2015 American Heart Association guidelines update for CPR and ECC. American Heart Association. 2015;1–32.
4. Hasegawa T, Daikoku R, Saito S, Saito Y. Relationship between weight of rescuer and quality of chest compression during cardiopulmonary resuscitation. *Physiological Anthropology*. 2014;33(16):1–7.
5. Idris AH, Guffey D, Aufderheide TP, Brown S, Morrison LJ, Nichols P, et al. Relationship between chest compression rates and outcomes from cardiac arrest. *Circulation* [Internet]. 2012 Jun 19 [cited 2016 Sep 25];125(24):3004–12. Available from: <http://www.pubmedcentral.nih.gov/articlerender.fcgi?artid=3388797&tool=pmcentrez&rendertype=abstract>
6. Monsieurs KG, De Regge M, Vansteelandt K, De Smet J, Annaert E, Lemoyne S, et al. Excessive chest compression rate is associated with insufficient compression depth in prehospital cardiac arrest. *Resuscitation* [Internet]. European Resuscitation Council, American Heart Association, Inc., and International Liaison Committee on Resuscitation.~Published by Elsevier Ireland Ltd; 2012 Nov [cited 2016 Sep 26];83(11):1319–23. Available from: <http://www.ncbi.nlm.nih.gov/pubmed/22828356>
7. Graham R, Coy MAM, Andrea M Schultz. Strategies to improve cardiac arrest survival a time to act [Internet]. Washington DC: the national academies press; 2015. p. 1–456. Available from: www.national-academies.org

8. **Ruiz de Gauna S, González-Otero DM, Ruiz J, Russell JK.** Feedback on the rate and depth of chest compressions during cardiopulmonary resuscitation using only accelerometers. *PloS one* [Internet]. 2016 Jan [cited 2016 Sep 25];11(3):e0150139. Available from: http://www.pubmedcentral.nih.gov/articlerender.fcgi?artid=4773040&tool=pmcentrez&render_type=abstract
9. **Ateyyah KA, Cady CE, Poltrock JT, Pirrallo RG.** A novel use of a metronome in a dispatcher assisted cardiopulmonary resuscitation. *Prehospital emergency care: official journal of the National Association of EMS Physicians and the National Association of State EMS Directors* [Internet]. 2014 [cited 2016 Sep 25];19(1):131–4. Available from: <http://www.ncbi.nlm.nih.gov/pubmed/2542005>
10. **Chung TN, Kim SW, You JS, Cho YS, Chung SP, Park I.** A higher chest compression rate may be necessary for metronome-guided cardiopulmonary resuscitation. *The American journal of emergency medicine* [Internet]. 2012 Jan [cited 2016 Oct 18];30(1):226–30. Available from: <http://www.ncbi.nlm.nih.gov/pubmed/21208766>
11. **Darmawan, Yahya Adi, Ernawati.** Automatic code red : meningkatkan efisiensi kompresi dada. *Proceedings meningkatkan kualitas tenaga kesehatan melalui penelitian, pengabdian masyarakat, dan publikasi ilmiah*. 2016. p. 17–8.
12. **Darmawan RE, Sujianto U, Rochana N.** Kompresi dada manual menggunakan neo automatic code meningkatkan kedalaman kompresi dada : manekin trial. *Candles up date* 2017. Kediri, Indonesia; 2017. p. 12–6.
13. **Gauna SR De, González-otero DM, Ruiz J, Russell JK.** Feedback on the rate and depth of chest compressions during cardiopulmonary resuscitation using only accelerometers. *Plos One*. 2016;11(3):1–17.
14. **Field, Soar, Davies, Akhtar, Perkins.** The impact of chest compression rates on quality of chest compressions – a manikin study. *Resuscitation*. 2011;83(3):360–4.
15. **Perkins GD, Benny R, Giles S, Gao F, Tweed MJ.** Do different mattresses affect the quality of cardiopulmonary resuscitation? *Intensive care medicine* [Internet]. 2003 Dec [cited 2016 Dec 8];29(12):2330–5. Available from: <http://www.ncbi.nlm.nih.gov/pubmed/14504728>
16. **Jäntti H, Silfvast T, Turpeinen a, Kiviniemi V, Uusaro a.** Quality of cardiopulmonary resuscitation on manikins: on the floor and in the bed. *Acta anaesthesiologica Scandinavica* [Internet]. 2009 Oct [cited 2016 Dec 8];53(9):1131–7. Available from: <http://www.ncbi.nlm.nih.gov/pubmed/19388894>

ORIGINALITY REPORT

19%

SIMILARITY INDEX

13%

INTERNET SOURCES

13%

PUBLICATIONS

13%

STUDENT PAPERS

PRIMARY SOURCES

1

worldwidescience.org

Internet Source

2%

2

Chandra Bagus Ropyanto, Sumarsih ., Niken Safitri Dyan Kusumaningrum, Wahyu Hidayati. "Effects of Benson's Relaxation Technique on Nausea in Patients with Chronic Kidney Disease Undergoing Hemodialysis", KnE Life Sciences, 2019

Publication

2%

3

Submitted to Universitas Sebelas Maret

Student Paper

2%

4

Santoso Santoso, Rita Kartika Sari, Anggorowati Anggorowati. "THE REFLECTIVE SUPERVISION MODEL: AN EFFORT TO INCREASE NURSE JOB SATISFACTION", Belitung Nursing Journal, 2017

Publication

1%

5

www.signavitae.com

Internet Source

1%

6

Internet Source

1%

7

Andhika Sukma, Bakti Jos, Siswo Sumardiono. "Kinetic of Biomass Growth and Protein Formation on Rice Bran Fermentation Using ", MATEC Web of Conferences, 2018

Publication

1%

8

Submitted to University of Central England in Birmingham

Student Paper

1%

9

sc.edu

Internet Source

1%

10

Chiwon Ahn, Juncheol Lee, Jaehoon Oh, Yeongtak Song, Youngjoon Chee, Tae Ho Lim, Hyunggoo Kang, Hyunggoo Shin. "Effectiveness of feedback with a smartwatch for high-quality chest compressions during adult cardiac arrest: A randomized controlled simulation study", PLOS ONE, 2017

Publication

1%

11

Submitted to Universitas Diponegoro

Student Paper

1%

12

jphysiolanthropol.biomedcentral.com

Internet Source

1%

13

www.wjem.com.cn

Internet Source

1%

14	docplayer.com.br Internet Source	1%
15	journals.plos.org Internet Source	1%
16	fr.scribd.com Internet Source	1%
17	www.ensihoidontiedotus.fi Internet Source	1%
18	repository.unair.ac.id Internet Source	1%
19	Khalid A. Ateyyah, Charles E. Cady, James T. Poltrock, Ronald G. Pirrallo. "A Novel Use of a Metronome in Dispatcher-assisted Cardiopulmonary Resuscitation", Prehospital Emergency Care, 2014 Publication	<1%
20	www.ijme.net Internet Source	<1%
21	eprints.soton.ac.uk Internet Source	<1%

Exclude quotes On

Exclude matches Off

Exclude bibliography On