

# The Signal Processing of Heart Sound from Digital Stethoscope for Identification of Heart Condition Using Wavelet Transform and Neural Network

*by* Jatmiko Endro Suseno

---

**Submission date:** 30-Oct-2020 06:45PM (UTC+0700)

**Submission ID:** 1431142125

**File name:** 12.\_ICICOS\_IEEE\_2017.docx (124.06K)

**Word count:** 2057

**Character count:** 10439

# The Signal Processing of Heart Sound from Digital Stethoscope for Identification of Heart Condition Using Wavelet Transform and Neural Network

**Abstract-** The ordinary stethoscope that is called acoustic stethoscope can detect heart sound and plug in order to know their health condition. However, the doctor diagnostics result depends on sensitivity of his hearing and experience. Also it couldn't be saved as patient's medical history. Therefore, these research have designed and developed a digital stethoscope with modify from the ordinary stethoscope which can produce heart sound via audio and graphics also the result can be saved in computer memory with addition of heart condition identification. The advantages of this research are very cheap production, portable, produce audio and graphics data, able to data saving and identify patient heart condition. The digital stethoskop is built from the ordinary stethoscope using sensor of the condenser microphone for convert analog signal become digital signal. The next process is signal processing such as amplification and low pass filter where frequency region below of 940 Hz, cause the heart sound produce sound between 0 and 940 Hz. These hardware sistem connects to sound card in the computer or tablet for several process of display to monitor, sound to speaker, recording and identification of heart condition using neural network. All of these software processes uses matlab 2014.

The experiment showed the best network architecture is used at number of neuron in second layer with each layer of 75 neuron. This architec produce highest accuracy, the accuracy is 82,14 % and need learning time fast enough compare with another ones, time is 96 detik. And wavelet type that suitable is wavelet db3 with 10 decomposition level. highest accuracy to identify the heart condition with murmur aorta regurgitation and trikuspid regurgitation, of 100 %, then mitral reguritasi with accuracy of 83,3 %, mitral stenosis with accuracy of 75 % and lowest accuracy for normal heart with accuracy of 70 %.

**Keyword:** heart sound, stethoscope, digital, cheap, and identification

## I. INTRODUCTION


Nowdays, instrument to heart sound diagnosis is acoustic stethoscope. Mostly, medical doctors arround more than 90 % use stethoscope for patient diagnosis [1]. Heart with unnormal condition produces sound addition which called murmur [2]. The operation of ordinary stethoscope has several lack of diagnosis. The problems of the acoustic stethoscope usage are environment noise, low sensitivity, low amplitude and no variation of the sound patten. The diagnose's doctor depend on ear sensitivity's doctor and his experience. Another

disadvantgae is the heart sound can't save as heart history's patient and for matter of discussion by among doctors. Another word, conventional stethoscope is tool let behind and very inaccurate. Therefor, important thing to develop stethoscope become digital instrument. Recent, there are digital stethoscope, however it is still very expensive and can't save teh data's patients. In this research, we design and produce the smart digital stethoscope with some advantages such as very cheap production, portable, produce audio and graphics data, able to data saving and identify patient herat condition. Hence, this instrument can be used by all people to first diagnose before go to doctor to next diagnosis.

## II. THEORY

Heart sound produces two different sounds using stethoscope tools, there are sound of 'lub' and 'dubs'. The first sound (S1) or sound of 'lub' is caused by closing triskupid and mitral valves. The flood flows from auricle to chamber of heart and stop the opposite direction. The second sound (S2) or sound of 'dub' is produced at end of sistole and first of diastole, and is raised by closing aortic and pulmolic valves. The flood leaves heart to body and lungs .

Sounds of S1 and S2 are showed at figure 1 (a). The disease because heart valve can't work as usually. If valve can't open widely so only a little flood can flow it. Opposite, if valve can't close completely, so that flood can flow oppositely, which is like to show figure 1 (b).

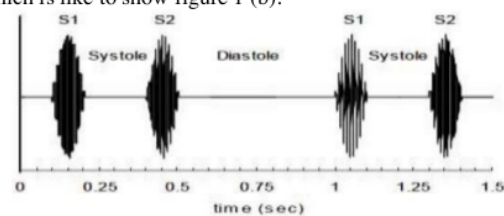

a.

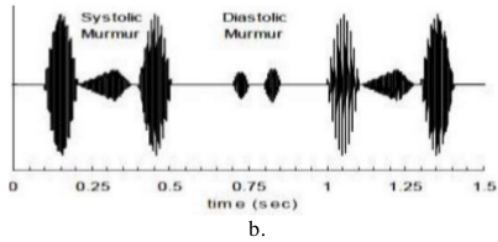


Fig. 1. The heart sound (a) normal and (b) with murmur [3]

Frequency range of the normal heart sound is between 20 Hz and 400 Hz. However, the frequency range of the abnormal heart is less than 1000 Hz. Murmur is sound that heard as continuously for periods of systolic, diastolic or the both. Murmur can be classified become murmur of systolic dan diastolic depend on the phases. [3]. Figure 2 shows some sample of murmur signals.

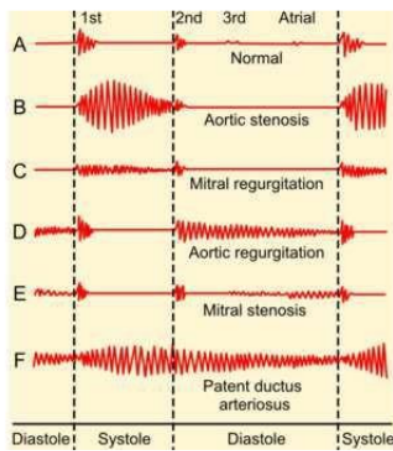


Fig. 2. The heart sound of normal and abnormal [4]

The murmur of systolic is sound that heard continuously between S1 and S2. The murmur of diastolic is sound that heard continuously between S2 and next S1. The early murmur diastolic awal starts from S2 and culminates at the first phase of three phases of diastole periode. This is because S2 is difficult to be heard, however S1 can be heard easily [4].

### III. METHODS

The design of the research instrument is used as recording process of the heart sound signal.

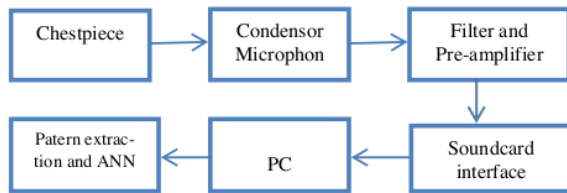


Fig. 3. Diagram block of the digital stethoscope design

The steps of the reasearch are:

1. Design of instruments such as chestpiece, microphone condensor, filter, dan pre-amplifier.
2. Display of graphics visual from the heart sound signal.
3. Recording process of the digital signal and activation of heart sound via computer speaker.
4. Data acusition from patient with variety heart condition.
5. Separate the signal graphics become a frame block for a heart sound.
6. Extract the signal characteristics from a heart sound periode using Wavelet Transformation with some processes, such as rectifying, enveloping, differentiation, dan thresholding.
7. Identification process of the heart sound using backpropagation neural network.

The data aqutition process starts from the chestpiece sensor placed at the patient's auscultation point. When the chestpiece sensor is affixed, the sound or the heart noise vibrates the chestpiece sensor, creating acoustic wave pressure propagating up to the rubber tube. Condenser microphones mounted on the ends of the rubber hoses are also covered by the acoustic waves. Sound waves coming into the microphone vibrate this diaphragm component. The diaphragm is placed in front of a disc and the arrangement of this element is formed capacitor. High low sounds coming into the microphone will cause variations from inside the space between the diaphragm and the backplate. This occurs because of the diaphragm movement relative to the backplate as a result of the pressure on the diaphragm. From the movement, an electrical signal will be generated which then goes to the filter. After the signal is filtered, the signal will be forwarded to the amplifier section. This amplifier circuit is a microphone pre-amplifier circuit that serves to amplify the input signal coming from the microphone before entering the laptop soundcard.

Research sample for heart that has murmur in patient in dr. Kariadi hospital. While for normal heart samples can be obtained from all respondents who heart normal. The type and number of samples for the heart that has murmurs depends on the patient's murmur patient in dr. Kariadi hospital. Each respondent will be recorded heart sound using a digital stethoscope. Recording will be done at all points auscultation, either on the respondent who have or not have murmurs.

In this study, heartbeat data aqutition was conducted for 18 seconds and produced 144000 data every 1 time the data retrieval process. Each recorded signal is captured / recorded one beat at 4 beats and the data size is equalized by data by using the command in the program

### IV. RESULT AND DISCUSSION

In this research, it is used low pass filter with frequency cut off 940 Hz, according to the heart sound frequency between 20 – 940 Hz. The process after filter, the signal will pass to pre-amplifier unit. The pre-amplifier unit function is to amplify input signal from microphone before to enter computer soundcard. The testing is gotten the signal response graphics can be seen at figure 4.

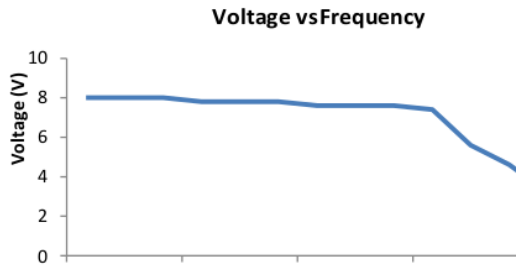


Fig. 4. The graph of signal response in low pass filter frequency

#### 4.1. Wavelet Transformation

Process of characteristics extraction for each the heart sound signal is done with some processes, such as rectifying, enveloping, differentiation, and thresholding. The process of wavelet transformation is done with convolution of signal with filter data. In the process, the input signal pass to two filters complemer (low-pass H dan high-pass G) dan down sampling with delete the second data, so that get coefficient approximation of cA

##### a. Rectifying

In rectifying process, the result of the heart sound signal is displayed in wave shape and be taken thge absolute number. The process is ocured in order to get no negatif data so that next process is easy. The result of rectifying process is showed at figure 5.

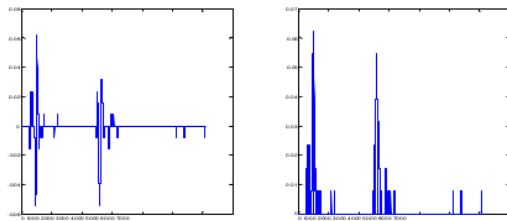


Fig. 5. Before and After Rectifying Process at Sound Graph of Normal Heart Sound

##### b. Enveloping

The enveloping process is process to get top data number from output of rectifying process, or another word, this process will take outer unit from the heart sound signal which recorded from output of rectifying process.




Fig. 6. The Enveloping Process

This process uses wavelet transformation. The input signal is decomposed using the daubechies wavelet method. This

research used db3 and db6 with each wavelet process using 7 and 10 decomposition levels.

##### c. Differentiation

The differention proses will be looked for the steep lines from each outpu enveloping data with calculate gradiens position.

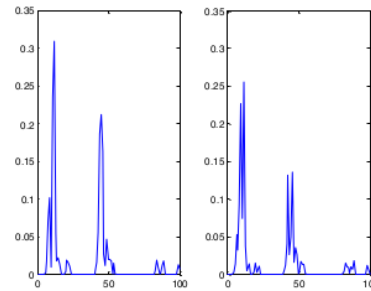


Fig. 7. The Differentiation Process

##### d. Thresholding

The thresholding process is to more feature of specifics characteristics from input signal with give treshold number. This research was used treshold number of 0,15.

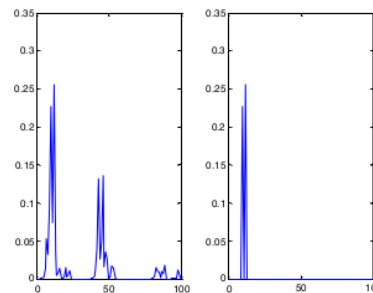


Fig. 8. Graphics of tresholding output

The output of this process is the fature of signal

#### 4.2. Network Architecture

The artificial neural network is design using backpropagation method. The network layers include layers of input, hidden, and output. With variation of neuron number in hidden layer with two layers of the hidden unit, also usage logsig method as the activation function. The epoch adjust 15000 and error target is 0,001. The results of the neural network can be showed at table I.

TABLE I  
Result of Neural Network with 2 hidden layer

Wavlet Type	Dekomposition Level	Number of neuron	Time (s)	Training Accuracy (%)	Testing Accuratio n (%)
Db3	7	100 (layer1)	125	88,04	39,29
		50 (l layer 2)			
Db3	7	75 (layer 1)	144	89,13	42,86
		75 (layer 2)			
Db3	7	50 (l layer 1)	103	89,13	46,43

		100 (layer 2)			
Db6	7	100 (1 layer 1)	111	86,96	42,86
		50 (layer 2)			
Db6	7	75 (layer 1)	116	86,96	46,43
		75 (layer 2)			
Db6	7	50 (layer 1)	115	85,87	57,14
		100 (layer 2)			
Db3	10	100 (layer 1)	89	96,74	75
		50 (layer 2)			
Db3	10	75 (layer 1)	96	96,74	82,14
		75 (layer 2)			
Db3	10	50 (layer 1)	93	96,74	75
		100(layer 2)			
Db6	10	100(layer 1)	101	93,48	78,57
		50(layer 2)			
Db6	10	75 (layer 1)	116	96,74	75
		75 (layer 2)			
Db6	10	50(layer 1)	132	98,91	78,57
		100 (layer 2)			

and tricuspid regurgitation with accurations of 100 %. However, lowest accuration is normal with accuration 70 %.

From table I, the best network architecture is used at number of neuron in second layer with each layer of 75 neuron. This architec produce highest accuration, the accuration is 82,14 % and need learning time fast enough compare with another ones, time is 96 detik. And wavelet type that suitable is wavelet db3 with 10 decomposition level.

TABLE II  
Result of testing accuration

Heart Condition	Number of testing data	Correct data	Accuration (%)
Aorta regurgitation	4	4	100
Tricuspid regurgitation	4	4	100
Mitral stenosis	4	3	75
Mitral regurgitation	6	5	83,3
Normal	10	7	70

From table II, we can know that the network architecture have highest accuration to identify the heart condition with murmur aorta regurgitation and trikuspid regurgitation, of 100 %, then mitral reguritation with accuration of 83,3 %, mitral stenosis with accuration of 75 % and lowest accuration for normal heart with accuration of 70 %.

#### V. CONCLUSION

The research have been developed instrumentation of digital stethoscope which can identify heart condition's patient. The instrument accuration is 82,14 %. Types of heart condition's patiens are aorta regurgitation, tricuspid regurgitation, mitral stenosis, mitral regurgitation, and normal. Highest accurations are identifications of aorta regurgitation

# The Signal Processing of Heart Sound from Digital Stethoscope for Identification of Heart Condition Using Wavelet Transform and Neural Network

---

## ORIGINALITY REPORT

---

2%

SIMILARITY INDEX

1%

INTERNET SOURCES

1%

PUBLICATIONS

1%

STUDENT PAPERS

---

## PRIMARY SOURCES

---

1

"Program schedule", 2017 1st International Conference on Informatics and Computational Sciences (ICICoS), 2017

Publication

1%

2

[id.123dok.com](http://id.123dok.com)

Internet Source

<1%

---

Exclude quotes Off

Exclude matches Off

Exclude bibliography Off